BIODENSIFICATION




REFRIGERATE PRODUCT UPON ARRIVAL

- Ready to use
- No mixing required

STORAGE

Product will be shipped in an insulated shipping box and/or with cold packs, which may thaw during shipment. If the gray temperature indicator located on the product packaging is **black** upon arrival, the efficacy of the graft material may have been compromised. Please contact SteinerBio immediately for instructions to replace the products: (866)317-1348

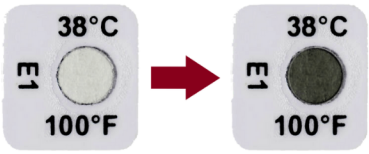

NOTIFY US IMMEDIATELY IF TEMPERATURE DOT IS BLACK

DIRECTIONS

- After creating the osteotomy, place BioDensification into the osteotomy and slowly drive the implant into the osteotomy. The implant will force the graft material into the surrounding bone.
- For "spinners" during implant placement, remove the implant and place BioDensification into the osteotomy, then reinsert the implant. BioDensification will stabilize the implant and improve the potential for implant integration.

PRECAUTIONS

BioDensification is indicated for use in osteotomies that have all walls remaining. In cases where a significant portion of the osteotomy is missing, ridge augmentation surgery may be required. Do not overfill the osteotomy. Do not leave defect open. Do not compromise blood supply to the defect area. This product has not been studied in pediatric patients. Do not mix with any other graft materials other than SteinerBio bone grafts.

Federal law restricts this device to sale by or on the order of a dentist.

BIODENSIFICATION

DESCRIPTION

BioDensification is a dual phase calcium phosphate based synthetic bone graft material. This product is designed to be quickly and completely resorbed, and to produce normal, healthy vital bone. This product contains no human or animal tissue.

INDICATIONS

BioDensification is a bone grafting material intended for use in poorly mineralized bone where the osteotomy has all walls remaining.

CONTRAINDICATIONS

This product is contraindicated in individuals who are unable to follow post-op instructions.

WARNINGS

BioDensification is single use only. Do not re-sterilize or reuse.
Do not use BioDensification if the package has been opened or damaged, or has exceeded the expiration date. Do not use if the temperature indicator on the packaging has turned black.

STEINERBIO
1051 Olsen St., Bldg 3611
Henderson, NV 89011
contactus@steinerbio.com
www.steinerbio.com
866.317.1348